


Jodi®- XL

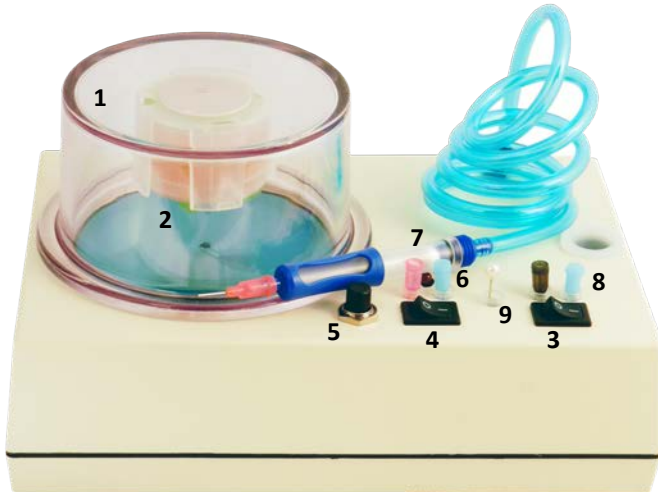

1. Desiccator Lid- *keep o-ring contact area clean*
2. Desiccant - *green= wet, orange= dry*
3. Vacuum On/Off Switch
4. Desiccator On/Off Switch
5. Vacuum Release *remember- turn off switch #4*
6. Vacuum Chamber Indicator Light
7. Vacuum Filter with Ball - **please don't clean, they can be filled up and then replaced inexpensively**
8. Inserts for Needle Storage (four of them)
9. Shallow Insert for Reamers

1. Turn on switch (#3) to Vacuum, use needle vacuum (#7)

The White ball in the filter is an air flow indicator. When air is flowing through the needle past the filter, it pushes the ball towards the tubing on its way to the vacuum pump. If the air stops flowing, the ball drops away from the tubing.

Please clean the needle first as the filter takes a long time to fill up with debris. Clean the needle while the vacuum is running, insert reamer into needle to push lodged wax into filter.

DESICCATOR

1. Place desiccant into holder on lid (**the imprinted words "DRY TOP" Towards Lid...to Recharge" facing you**)
2. Place hearing instruments on plate, DO NOT COVER HOLE IN CENTER OF PLATE, REMOVE BATTERIES AND SOFT EARMOLDS.
3. Place lid (#1) over CLEAN o-ring.
4. Turn on switch #4, vacuum pump will engage removing air from the chamber, indicator light will turn on, heater will start and the vacuum pump will automatically shut off when vacuum is reached.
5. To remove hearing instruments, turn off electrical switch (#4), push vacuum release button (#5) and hold down until all vacuum is removed, lift lid and remove hearing aids.

HELPFUL HINTS

1. Turn on desiccator with lid in place first thing each morning to pre-heat plate making it ready for immediate use and leave on all day. Heater is completely fireproof. The plate requires 15-20 minutes to reach an approximate temperature of 105 degrees. Follow step #5 to put hearing aids in desiccator.
2. The desiccator @ 105 degrees with a dry (orange) desiccant will remove two drops of water in approximately 20 minutes. **Open battery doors, control doors, remove ear hooks where possible, prior to placing hearing aids in desiccator.**
3. Desiccant (#2) When crystals turn green, rejuvenate in a microwave oven for 30 second intervals, on a high setting for 750-1250 Watt, over 1250- 15 second intervals, until they turn orange. Wrap paper towel around desiccant to absorb moisture during drying process. **Desiccant plastic container can get very hot when drying in microwave, hot enough to melt, hot enough to burn you.**

4. Our pink needle is specifically designed for maximum vacuum efficiency in CIC's, ITC, ITE, and RIC sound bores.

The Light Blue needle is sized for open ear Thin Tubes.

Our Black needle is oversized for Ear Molds.

Use of force will bend these needles and ruin Hearing instruments.

Changing this needle to another size will decrease vacuuming efficiency in the sound bore and the receiver nubbin.

CLEANING

DO NOT IMMERSE IN LIQUIDS OR APPLY LIQUIDS BY POURING ONTO UNIT.

FIRST—Test your preferred cleaning product on a small area.

Alcohol or household ammonia is very effective.


TROUBLESHOOTING

If the desiccator pump recycles too often, there is a vacuum leak; most likely due to debris on O-ring or Lid surface.

Remove the lid from the plate, turn on the desiccator switch (#4) Wet your finger and place it firmly over the center hole. The pump should shut off and stay off as long as your finger remains firmly over the hole. If the pump recycles, please call customer service.

If the pump shuts off and stays off, clean the o-ring . Inspect the bottom rim of the lid (#1) where it meets the o-ring for debris, cracks, or dents.

Still need help? Call Kat in customer service. kat@jodivac.com • 503-774-4951 • Toll Free 866-856-5634

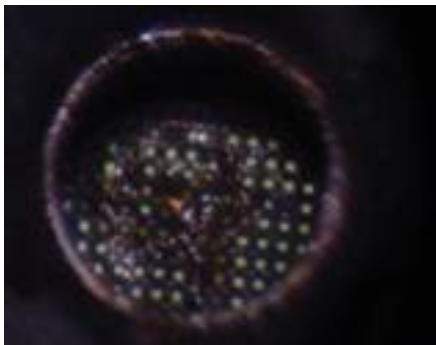

Receiver Screen with some debris.

A light is behind the holes to better show the openings.

Note: a Video Otoscope will not Amplify adequately to distinguish a clear hole verses an oil filled hole

Oil will block sound waves.

Hearing Aid Tech. Notes

Dear Professional,

Hearing Instrument design forces us to use a small needle, therefore it is important to understand that my needle is highly efficient and use of other "milled needles" will dramatically reduce its ability to pull debris through.

When removing Cerumen, remember it comes in many textures:

Hard and Dry, in all sizes and shapes– Best picked and vacuumed. Large pieces will sit on end of needle, remove from tip of needle.

Soft and Sticky – Slowly vacuum till clean

Oily- Vacuum till clean, then you may need to add a grease cutting agent to penetrate the small holes of the damped receiver screen as shown. Then vacuum the screen and repeat two more times to get all the holes cleared of oil.

Clear Non Sudsing Ammonia is excellent Cerumen emulsifier.

A single drop of ammonia dispensed from a size 20 needle is enough to liquefy this very small area.

Heads up — the more ammonia you introduce into the filter, the shorter the life of the filter. There is an optional liquid filter available.

Observation under a microscope:

Alcohol did not alter Cerumen, got it wet.

Hydrogen Peroxide also did not alter Cerumen, but rather made bubbles which moved particulates around. Emulsion did not take place.

Clear Non-Sudsing Ammonia turns Cerumen into a "bean soup" which dramatically improves the cleaning process.




1- Spare Filter

1- Blue Needle and Reamer

1- Reamer for Pink and Black

1- Pink Needle

1- Black Needle

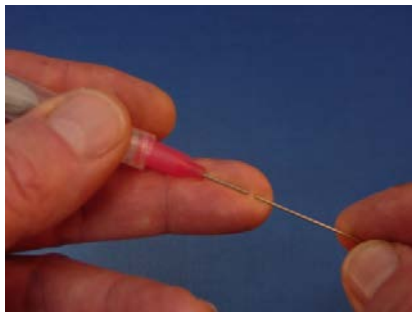

USING REAMER

Create an indent on your finger with needle, place reamer in the indent and slide into needle.

NOTES

- A plugged needle will cause flow indicator ball NOT to rise.
- A plugged needle will act as a ramrod and push wax deeper.
- Pushing needle in too fast without paying attention will produce undesired results.
- Pushing too hard on Microphone will dislodge Mic. from faceplate.
- Old Receiver tubes are prone to coming loose, be gentle.



Insert tubing past the locking teeth and continue pushing till tubing bottoms out.

To release push down black ring and hold while pulling tubing out
This quick release allows for easy tube replacement or to switch to the optional liquid filter.



READ ALL INSTRUCTIONS BEFORE USING IMPORTANT SAFEGUARDS

*THIS PRODUCT IS INTENDED FOR THE CLEANING OF HEARING AID DEVICES
AND NOT TO BE USED TO CLEAN EARS.*

DANGER – to reduce the risk of electric shock:

1. Always unplug this product immediately after using.
2. Do not use while bathing.
3. Do not place or store product where it can fall or be pulled into a tub or sink.
4. Do not place in or drop into water or other liquid.

WARNING – To reduce the risk of burns, electrocution, fire or injury to persons:

1. **Do not get the syringe end near eyes or ears, as the needle can puncture skin.**
2. **Do not clean ears with this product.**
3. **If your product comes with a Desiccant, and you are drying it out by use of a heating source— understand that the desiccant will get very hot and will burn your skin.**
4. **This product is intended to clean hearing aids, any unauthorized use will void any and all warranties.**
5. A product should never be left unattended when plugged in.
6. Close supervision is necessary when this product is used by, on, or near children or invalids.
7. Use this product only for its intended use as described in this manual. Do not use attachments not recommended by the manufacturer.
8. Never operate this product if it has a damaged cord or plug, if it is not working properly, if it has been damaged, dropped into water. Return the product to the manufacturer for examination and repair.
9. Keep the cord away from heated surfaces.
10. Never use while sleepy or drowsy.
11. Do not use where aerosol (spray) products are being used or where oxygen is being administered.

CAUTION — RISK OF ELECTRIC SHOCK, DO NOT REMOVE COVER. REFER SERVICING TO QUALIFIED PERSONNEL

This product is for use on a nominal 12VDC circuit. Use the appropriate AC to DC adapter as supplied with this product when plugging in to household current. This product is factory equipped with a specific electric cord and plug to permit connection to a proper electric circuit. Make sure that the product is connected to an outlet having the same configuration as the plug. Do not modify the plug provided – if it will not fit the outlet, have the proper outlet installed by a qualified electrician. If the product must be reconnected for use on a different type of electrical circuit, the reconnection should be made by qualified service personnel.

WARRANTY

If wax or debris is found inside unit, it will be assumed that vacuuming occurred without the protection of the supplied filter assemblies. Please do not clean filter assemblies. Replacement filters are available. A \$30.00 cleaning charge may be applied.

Manufacturer will repair or replace the product for all defects and workmanship for a period of 3 Years from the date of purchase.

Syringe assembly and needle are excluded from this or any other warranty.

Manufacturer is not responsible for incidental or consequential damages arising from accident, abuse, misuse, or failure to follow instructions for the product. Any alteration of the product voids this warranty.

To activate this warranty, purchaser must show proof of purchase date of the product. If purchased through JodiVac, your warranty will be automatically activated.

Purchaser is responsible for shipping and handling costs when returning the product for warranty service.

SERVICE

JodiVac LLC
17912 SE Mill Court
Portland, OR 97233

Contact: Kat
Toll Free 866-856-5634
Voice 503-774-4951

kat@jodivac.com
Fax 503-287-8408